

# Load Cell Central

1-800-LOADCEL

## OM - 10



### FEATURES

- Complete Strain Gage Bridge Signal Conditioner
- Isolated 10 Volt Output
- Bridge Balance with 80% Tare Offset Capability
- Excitation Supply Capable of Driving Four Load Cells
- AC Powered
- Rugged Epoxy Encapsulated Design


### APPLICATIONS

- Weighing with Load Cells
- Low frequency strain measurements
- Process Control Pressure Transducers
- Can Be Used With All Types of Low Output Sensors

### DESCRIPTION

The Model OM-10 is a self contained, AC powered signal conditioner for bridge type instrumentation. It contains a precision instrumentation amplifier with isolated, filtered output and a highly regulated, low noise, adjustable output bridge excitation source. The unit is completely encapsulated for use in rugged environments.

### BLOCK DIAGRAM

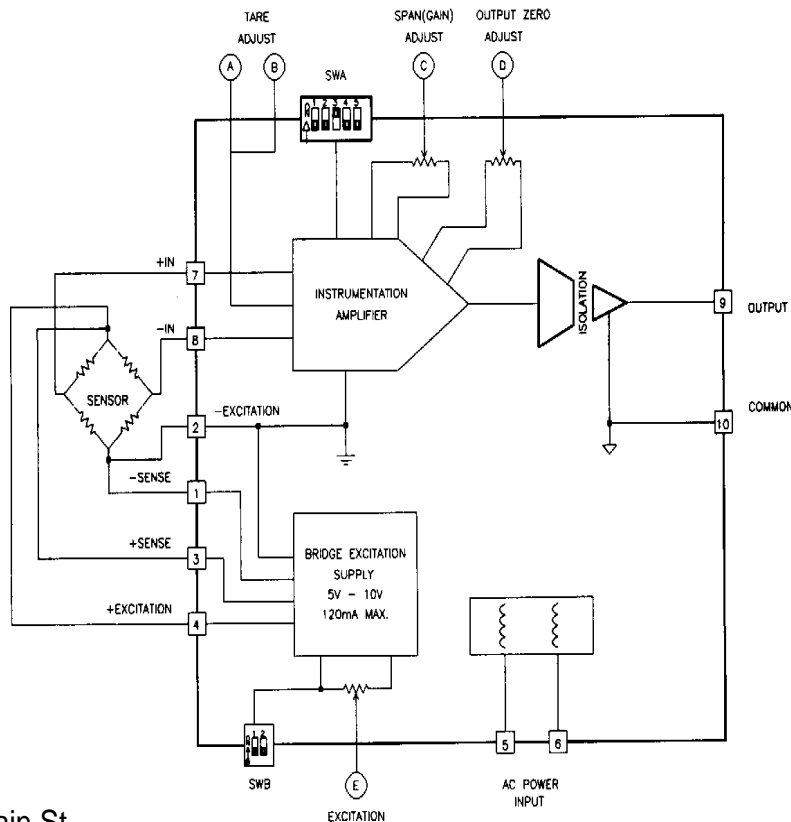

Load Cell Central  
 P. O. Box 91 / 216 Main St.  
 Monroeton, PA 18832  
 Toll Free: 1-800-LOADCEL / 1-800-562-3235

Phone: 1-570-265-5015  
 Fax: 1-570-265-5148  
 Email: salesam@800loadcel.com  
 Web: www.800loadcel.com

## SPECIFICATIONS

NOTE: Unless otherwise noted, specifications apply after 1 hour warm up at 25°C ambient.

Temperature Coefficients apply between 0°C and 55°C ambient.

ISOLATION	
Input to Output	700 VDC 60pF
AMPLIFIER	
GAIN	
Adjustment Range	200 to 2000
Input for 10V Output	5 mV to 50 mV
Linearity	±0.005% of Full Scale
Temperature Stability	50 PPM (0.005%/°C)
INPUT NOISE	
.1 Hz to 10 Hz	2µV P-P
INPUT OFFSET	
Temperature Coefficient	0.5µV/°C typical
TARE ADJUSTMENT RANGE	
Bridge Balance	-3mV to +25mV
Referred to Input	Equals 80% F.S. of 3mV/V cell
Temperature Coefficient	1µV/°C typical
INPUT RESISTANCE	
Differential and Common Mode	1000 megohm
COMMON MODE REJECTION	
DC to 60Hz	90 dB minimum
COMMON MODE INPUT	
	0 to +5 Volts maximum
OUTPUT	
ZERO ADJUST	
	0 or +2 Volts
Temperature Coefficient Referred to Output	0.3mV/°C typical
OUTPUT VOLTAGE RANGE	
	-3 to +10 Volts
Current	5 mA maximum
Frequency Resonse, -3dB	10 Hz, 2 pole
Response Time	
Rise Time 10% to 90%	35 ms
To 0.1% of Final Value	100 ms
BRIDGE SUPPLY	
VOLTAGE ADJUSTMENT RANGE	
	5 to 10 Volts
Temperature Coefficient	100 PPM typical
Fixed	10.2V ±2.5%
Temperature Coefficient	60 PPM typical
LOAD CURRENT	
	0 to 120 mA
REGULATION - LOAD & LINE	
	0.02% maximum
OUTPUT NOISE	
120 Hz Bandwidth	1 mV RMS, maximum
POWER INPUT	
	115 VAC, ±10V 50/60 Hz @ 6 VA
Optional	100, 220 or 230 VAC, ±10%
LINE ISOLATION	
Capacitance	60 pF typical
Dielectric Withstand	1100 Volts RMS
ENVIRONMENT	
Ambient Operating	-25°C to +55°C
Storage	-25°C to +85°C
WEIGHT	
	18 oz. (510 grams)
SIZE	
	3.75" L x 2.0" W x 3.0" H (9.53 cm x 5.1 cm x 7.62 cm)

## GETTING STARTED WITH THE MODEL OM-10

1. Excitation Supply: If remote sensing is not used, connect +Sense to +Excitation, terminal 3 to 4, and connect -Sense to -Excitation, terminal 1 to 2. These connections must be made to adjust the supply as in step 2.
2. Apply power to the Model OM-10 and adjust the Excitation supply. Turn SWB-1 "ON" for a fixed 10 Volts. This will set the supply to 10.2 ±2.5% and provide the best temperature stability. For voltages between 5 and 10 Volts, place SWB-1 in the "OFF." position and set the Excitation Supply with potentiometer E. SWB-2 may be in either position.
3. Turn the power to the Model OM-10 "OFF" and connect the load cell to the Model OM-10 Excitation terminals and the Amplifier Inputs.
4. Turn on power to the OM-10.
5. Turn SWA-3 "ON". (To set output ZERO)
6. Select the expected full scale signal range according to the table with SWA-4 and SWA-5. If the output from the load cell is not known, set both SW-4 and SW-5 "ON" for the 40-50mV range.
7. Select required ZERO output range. SWA-2 "ON" for zero Volts or SWA-2 "OFF" for +2 Volts.
8. Adjust D potentiometer for 0 or +2 Volts.
9. Turn SWA-3 "OFF". Expect output to change.
10. Apply no load or dead weight to load cell.
11. Adjust TARE potentiometers A and B for the same ZERO output set in Step 8. SWA-1 "OFF" provides a bridge output balance of -3mV to +15mV, and "ON" between +15mV and +25mV, referred to the amplifier input. This adjustment does not change the output of the bridge.
12. Apply full scale load and adjust SPAN (GAIN) potentiometer C for the desired full scale output. Set Range switches SWA-4 and SWA-5 as required.
13. Remove full scale load and check ZERO output. Adjust FINE TARE potentiometer A if required.
14. Recheck full scale as in Step 12.
15. End.

Note: If the amplifier is used without using the OM-10 Excitation Supply, the external power supply low side must be connected to the -EXCITATION pin 2 on the Model OM-10, or one of the inputs must be tied to pin 2, -EXCITATION. This provides a DC return path for the finite amplifier input current.

## AMPLIFIER

The amplifier is a true differential input, low drift Instrumentation Amplifier with less than 100pA input current. It has a common mode range of 5 Volts with respect to the - EXCITATION supply terminal and a minimum of 90dB rejection of the common mode voltage. The input amplifier and excitation supply are DC isolated from the AC line and the output.

## TARE WEIGHT COMPENSATION

The Model OM-10 has two different zero controls. One is called the OUTPUT zero and can be set to 0 Volts or + 2 Volts with SWA-2. The other zero control is called TARE. SWA-1 allows the selection of one of two TARE ranges, -3mV to 15mV or +15mV to +25mV. Potentiometers are available for COARSE and FINE TARE adjustments.

## CONNECTING TO A SENSOR


Any amplifier has a finite input current which must have DC return path to the amplifier power supplies. This path is automatically provided when the Model OM-10 Bridge Excitation Supply is used to excite the sensor. If an external supply is used, one side of the external supply must be connected to the Model OM-10 -EXCITATION, Terminal 2. Be sure that the common mode voltage limits are observed. This would generally limit the external power supply to 10 Volts assuming that half the voltage would be common mode, as is the case when exciting a full bridge.

When the full scale output of a sensor is measured in millivolts, say 10 millivolts, care must be exercised in wiring systems. At 10 millivolts full scale, each microvolt ( $10^{-6}$  Volts) contributes 0.01% of full scale output. Wire connections can generate microvolts of potential due to contact potentials. These will also be thermoelectric potentials and thus vary with temperature differences. All wires used in connecting up the Model OM-10 should be of the same material. If any intervening connections are made such as a terminal block, the terminal block connecting points should have good thermal contact so they will always be at the same temperature and thus cancel each other.


## TRANSDUCER EXCITATION

The bridge excitation supply voltage is set by SWB-1 and potentiometer E. Set SWB-1 ON for a fixed 10 Volts. This will provide the best temperature stability. The supply can be adjusted between 5 and 10 Volts by setting SWB-1 OFF and adjusting potentiometer E. The supply will deliver up to 1 20mA current at any voltage setting to power up to four 350 ohm sensors.

ON FOR FIXED 10V EXCITATION      NOT USED



SWB-1	EXCITATION VOLTAGE
ON	FIXED 10 VOLTS
OFF	ADJUSTABLE

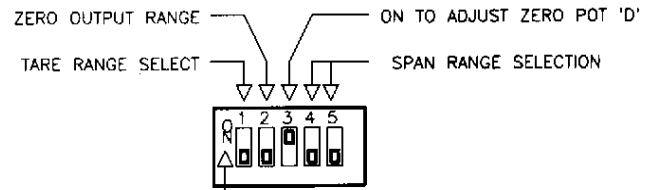


SWA-1	TARE RANGE
OFF	-3mV to +15 mV
ON	+15 mV to +25 mV


SWA-2	ZERO VOLTAGE
OFF	+2 V
ON	0 V

SWA-4	SWA-5	SPAN RANGE
ON	ON	40 mV to 50 mV
OFF	ON	20 mV to 40 mV
ON	OFF	10 mV to 20 mV
OFF	OFF	5 mV to 10 mV

## CASE DIMENSIONS

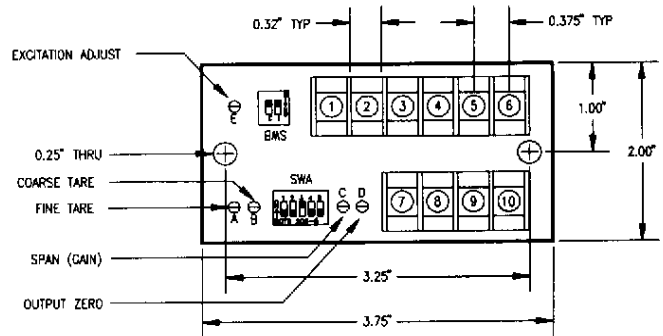

TOP VIEW

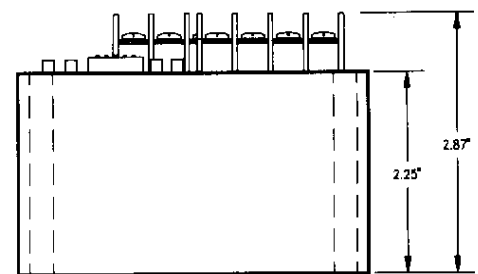

SIDE VIEW

TERMINAL STRIP ASSIGNMENTS			
SCREW TERMINAL	FUNCTION	SCREW TERMINAL	FUNCTION
1	-SENSE	6	AC
2	-EXCITATION	7	+SIGNAL
3	+SENSE	8	-SIGNAL
4	+EXCITATION	9	OUTPUT
5	AC	10	COMMON